

EasyPlus mini MasterDriver™

Self-Monitoring Blood Glucose System

Quick Reference Guide

Inserting Batteries



1. Open the battery door of the meter by slipping the tab in the direction of the arrow.




2. Insert a battery and the meter beeps.



3. Put the battery door back in place and snap it closed. The meter turns on automatically.

Setting The Time and Date—First Time Use

Setting the current time and date in your meter is important if you intend to use the meter memory or if you want to download your results to a computer.

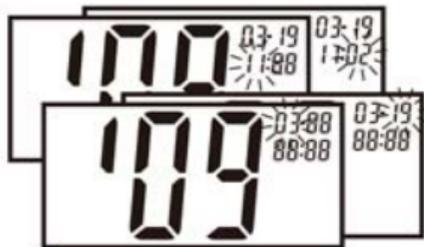


1. Insert a new battery, the meter beeps and turns on automatically.
2. The last 2-digits of the year flash at the center of the display. Press  to adjust the year and press  to confirm the setting.
3. Repeat step 2 to set the date and time. The flashing field is the one you are currently setting. When finishing the setting, the display shows **OK** and the meter beeps.

Running A Control Solution Test

You need the meter, a test strip, and control solution.




1. Put a test strip into the meter in the direction of the arrow.
2. The meter beeps and turns on automatically. The icon  and  shows itself.
3. Place the meter on a flat surface, like a table.
4. Remove the control solution bottle cap and wipe the tip of the bottle with a tissue.

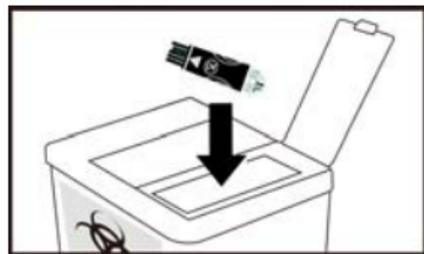


5. Squeeze the bottle until a tiny drop forms at the tip of the bottle.
6. Touch the drop to the Blood collection area at the tip of the test strip. **Do not put control solution on top of the test strip.** When you hear beeps, you have enough control solution in the test strip.
7. The meter starts to count down from 5 seconds, the display shows "Ok", and then shows the test result.
8. Do not remove the test strip yet. Check if the reading falls within the range printed on the test strip bottle.
9. Remove the test strip and throw it away after you have compared the reading to the range printed on the test strip bottle.

Inserting A Lancet Into The Lancing Device


You must first load the lancet into the lancing device to get it ready for use.

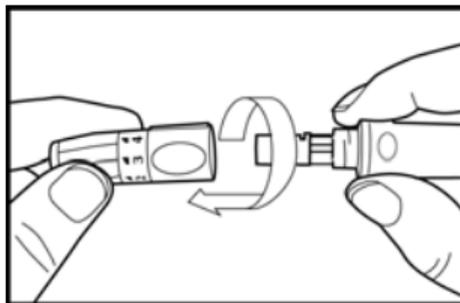

1. Unscrew the Cap.

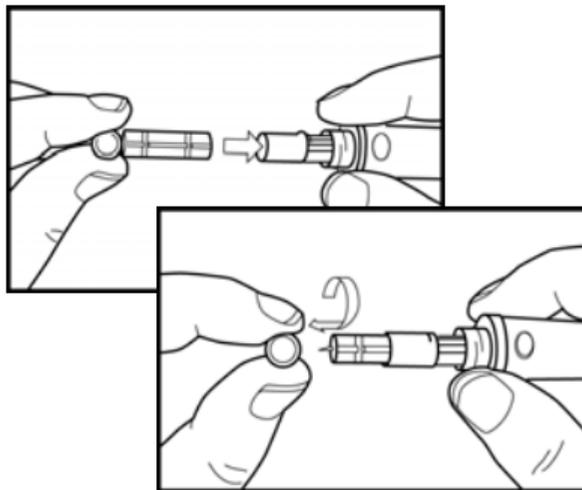


2. Insert the lancet into the lancing device firmly then twist off the protective cover.

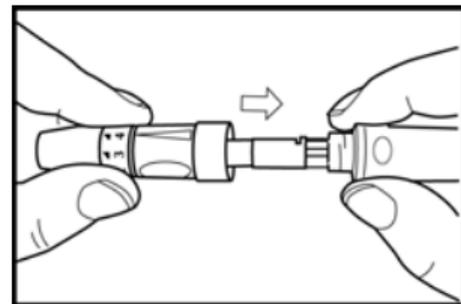


3. Recap the front cap.



Lancets are for use only and a new, sterile lancet should be used each time you perform a test.

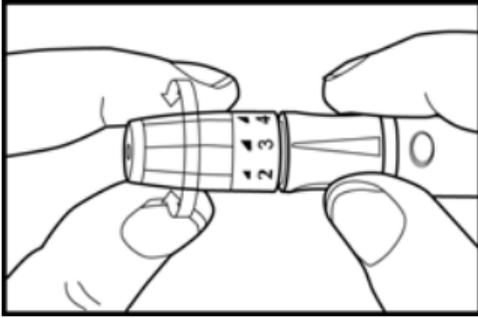


4. Select the desired penetration depth.

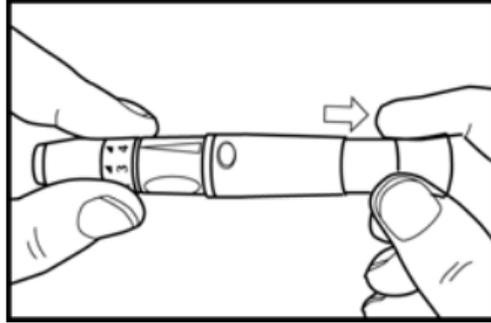

5. Pull on the sliding barrel of the lancing device until it clicks and then release.

Now the lancing device is ready.
Do not prick your finger until your meter and strip are prepared.

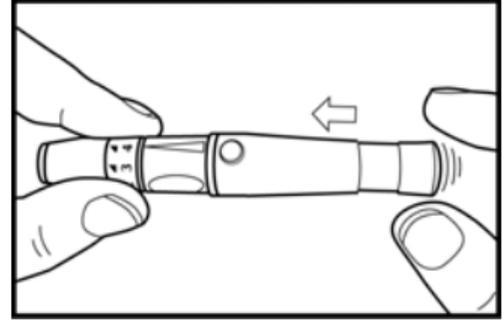


6. Set the lancing device aside until later in the test.



1. **Select 1-2 for soft or thin skin, 3 for average, and 4-5 for thick or calloused skin.**
2. **Lancing device and lancets are not to be shared between users. Sharing lancing devices and lancets may transmit blood borne pathogens, such as viral hepatitis.**


Running A Blood Glucose Test With Blood From Your Fingertip

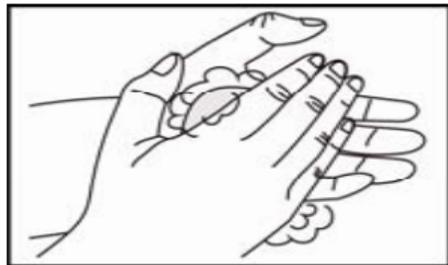


1. Wash your hands with soap and warm water.
Rinse and dry thoroughly.




2. Put a test strip into the meter in the direction of the arrow.
The meter beeps and turns on automatically.
3. When the blood drop flashes on the display, using the lancing device.

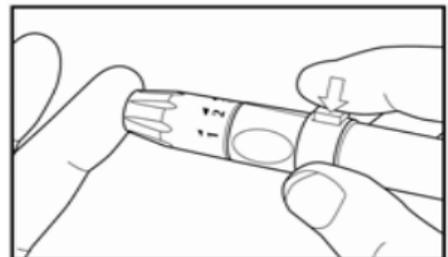

4. Hold the lancing device firmly against the side of your finger. Press the trigger button. Then remove the lancing device from your finger.

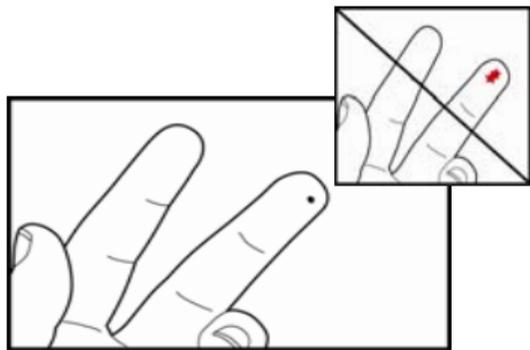

5. Gently squeeze and/or massage your fingertip until a round drop of blood on your fingertip.

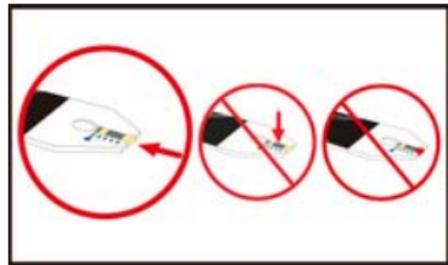

6. Touch the blood drop at the tip of the transparent window of the test strip. Do not put blood on top of the strip. When you hear beeps, you have enough control solution in the test strip.


Be sure to get enough blood in the test strip. Otherwise, an inaccurate reading may result.



7. The meter starts to count down from 5 seconds, the display shows "Ok", and then shows the test result.
8. Remove the test strip and the meter turns off automatically.

Running a Blood Glucose Test with Blood from Your Forearm


Please use the clear cap with the lancing device for AST testing.

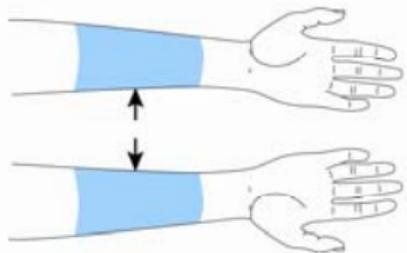

1. Massage the puncture area of forearm for a few seconds.




2. Press and hold the device with clear adjustable tip against the forearm.

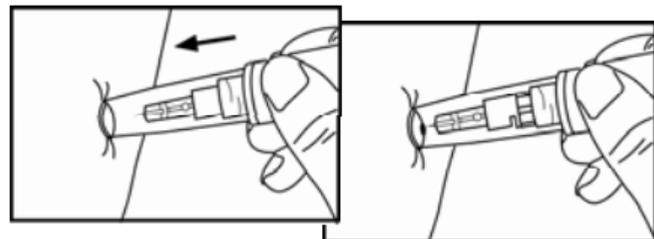


3. Press the trigger button to activate the lancing device.
4. Hold the device against forearm and increase pressure until the blood sample size is sufficient.


Running a Blood Glucose Test with Blood from Your Palm

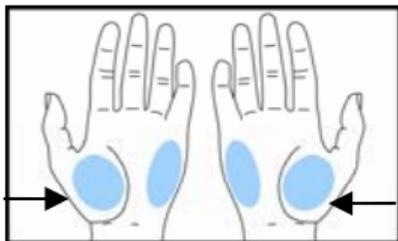

1. Massage the puncture area of palm for a few seconds.

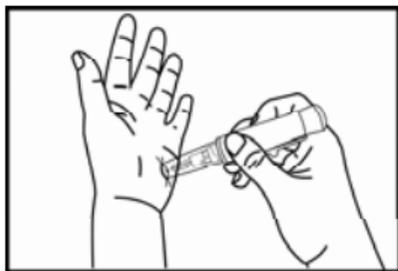

2. Press and hold the device with one clear adjustable tip against the palm.

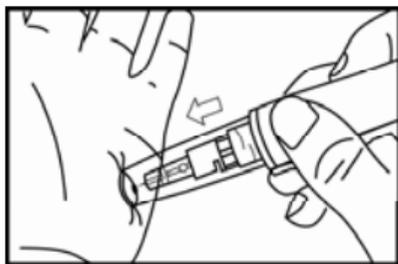


3. Press the trigger button to activate the lancing device.

4. Hold the device against forearm and increase pressure until the blood sample size is sufficient.




Check with your healthcare professional before testing other sites than fingertip.


Discarding Used Lancets

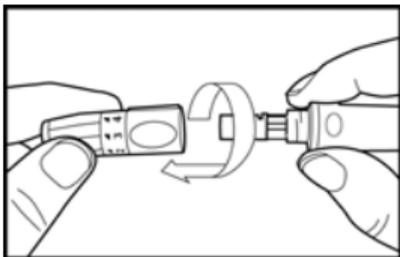

1. Unscrew and remove the cap.

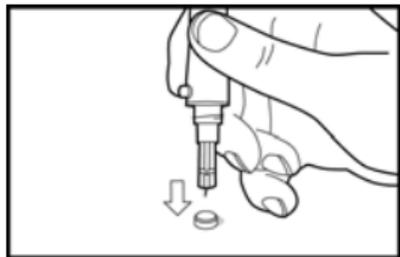

2. Without touching the used lancet, stick the lancet tip into its protective cover.

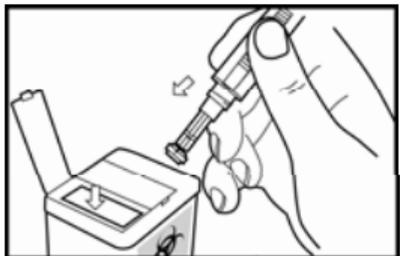


3. Pointing the lancing device toward a container for sharp or biohazard material, slide the ejection button down to release the covered lancet into the container.

Viewing & Deleting Test Results



1. Press  to turn the meter on.
2. Press  to enter memory mode. The meter shows the total number of the stored results first and then shows the latest result.

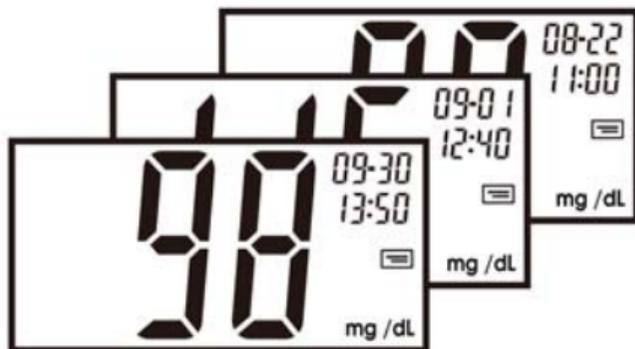

3. Press  to view the test result from latest to oldest.



4. To delete a test result, press  for 3 seconds. When display shows "dEL", press  to confirm the deletion.

Or press  to cancel the deletion and go back to the total number of the stored results.



5. Press  for 1 second to go back to the total number of the stored results.
6. Press  for 3 seconds to turn off the meter, or the meter turns off automatically in 90 seconds.

Screen Messages and Troubleshooting

Never make treatment decisions based on an error message. If you have any concerns, please contact your healthcare provider.

<i>Message</i>	<i>What it means?</i>	<i>What to do?</i>
	Humidified / Used strips The meter has detected a problem with the test strip.	Repeat the test with a new strip. Refer to pages 8-9 for information on sample application.
	Low power The meter batteries do not have enough power to perform a test.	Replace the new batteries.
	Volume detector error The volume of blood or control solution is NOT enough.	Replace with a new strip. If Err appears again, please contact your local dealer.

Message

What it means?

What to do?



Test result is higher than 630 mg/dL (35.0 mmol/L).

Re-check your glucose level. If the result is **HI** again, obtain and follow instructions from your healthcare professional without delay.



The test result is lower than 20 mg/dL (1.1 mmol/L).

This may require immediate treatment according to your healthcare professional's recommendations. Although this message could be due to a test error, it is safer to treat first and then do another test.



The meter is connecting to the computer.

You can start to use the embedded software. Please read **GlucoManager™ Data Management Software (GDMS)** User's Manual for more information.

Running With Your Computer



1. Plug the **EasyPlus mini MasterDriver™** meter into a USB port on your PC.

2. The display shows "PC" and the **GlucoManager™** software runs automatically.



For more information, please read **GlucoManager™ Data Management Software (GDMS) User's Manual.**



1. Make sure you had exited from **GlucoManager™** software, otherwise **DO NOT** plug out meter.
2. Do not insert strip while meter connect on PC.
3. The suggested monitor for the software is 1024 x 768 dpi.

P/N. 718039200_0375_02