


EG V1(BL)

Self-Monitoring Blood Glucose System


Quick Reference Guide

Setting The Time and Date—First Time Use


Setting the current time and date in your meter is important if you use the meter memory.

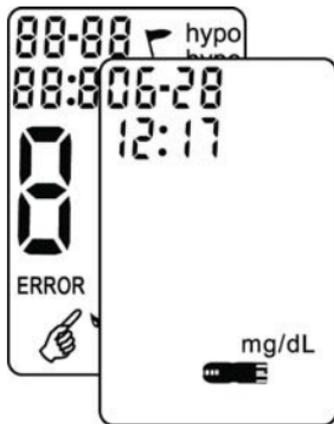

1. Press “▶” until turning the meter on.
Press “◀” once again and release to enter the setting mode.

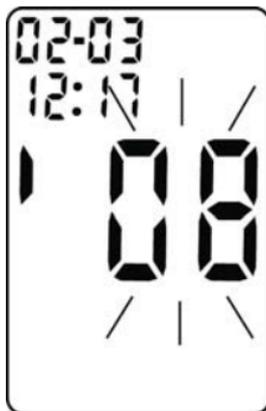

2. The last 2-digits of the year flash at the center of the display. Press “▶” to adjust the year and Press “◀” to confirm the setting.

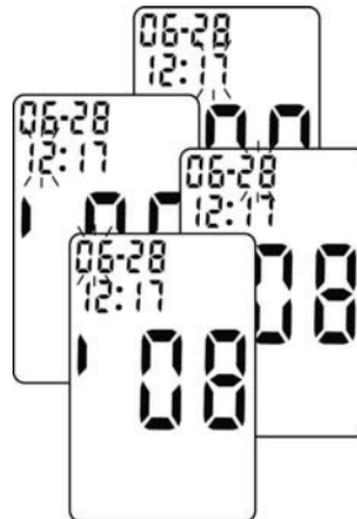


3. Repeat step 2 to set the date and time.
The flashing field is the one you are currently setting.


Setting Hypo and Hype



4. Press “▶” to adjust value of hypo and Press “◀” to confirm the setting.

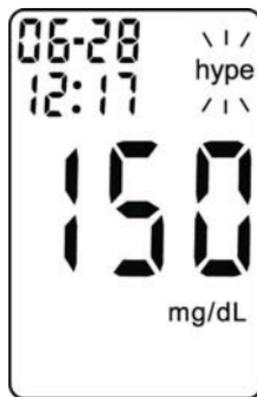

5. Press “▶” to adjust value of hype and Press “◀” to confirm the setting.


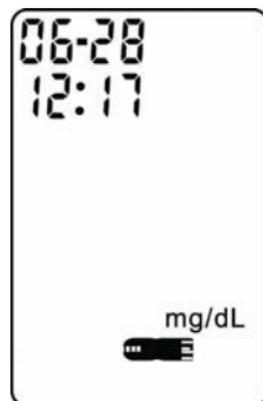


6. When setting is finished, the display will be back to the testing mode of flashing strip.



Hypo setting are from 60 to 80 mg/dL (3.3 to 4.4 mmol/L); Hype setting from 150 to 630 mg/dL (8.3 to 35.0 mmol/L).

Running A Control Solution Test

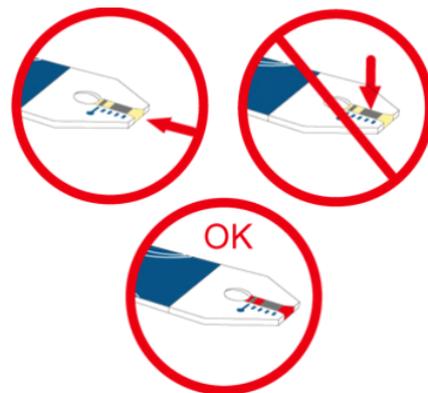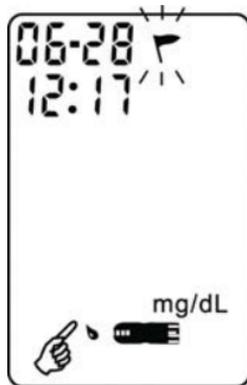

1. Put a test strip into the meter in the direction of the arrow.

2. Press “▶” for 1 seconds to set “▶”.

3. Place the meter on a flat surface, like a table.

4. Remove the control solution bottle cap and wipe the tip of the bottle with a tissue.

5. Squeeze the bottle until a tiny drop forms at the tip of the bottle.

Touch the drop to the Blood collection area at the end of the test strip.


Do not put control solution on top of the test strip.

When you hear the beeper, you have enough control solution in the test strip.

The meter starts to count down from 5 seconds and will show the results.




6. A result appears on the display.
Don't remove the test strip yet.
Check if the reading falls within the range
printed on the test strip bottle.

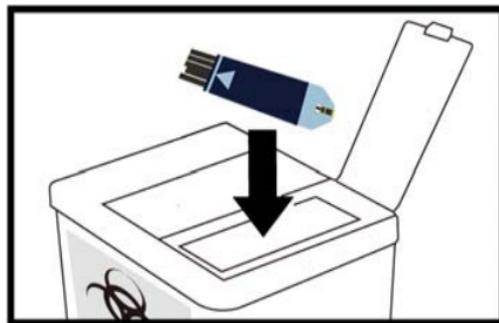



7. Remove the test strip and throw it away after
you have compared the reading to the range
printed on the test strip bottle.

Inserting A Lancet Into The Lancing Device


You must first load the lancet into the lancing device to get it ready for use.

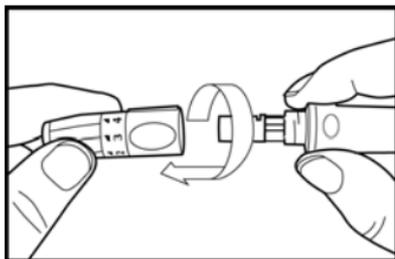

1. Unscrew the Cap.

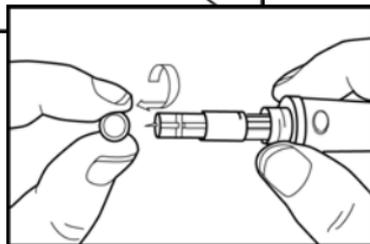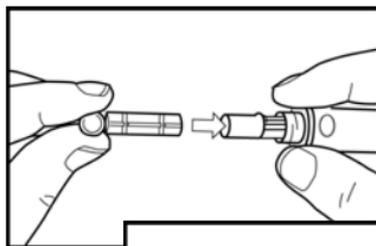


2. Insert the lancet into the lancing device firmly then twist off the protective cover.

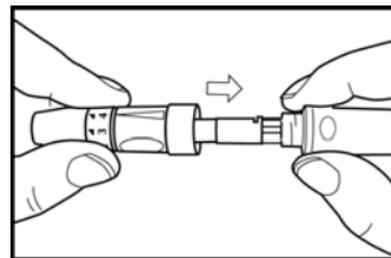


3. Recap the front cap.




Lancets are for use only and a new, sterile lancet should be used each time you perform a test.

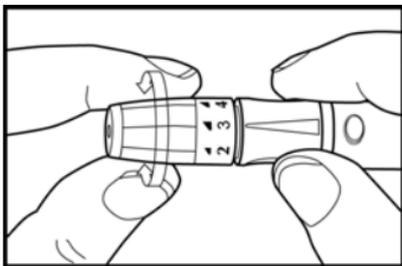

4. Select the desired penetration depth.

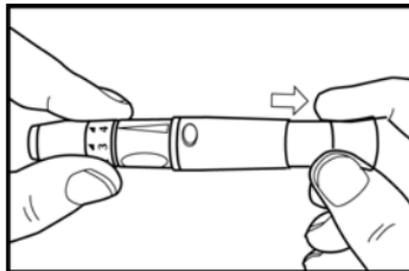

5. Pull on the sliding barrel of the lancing device until it clicks and then release.
Now the lancing device is ready.
Do not prick your finger until your meter and strip are prepared.

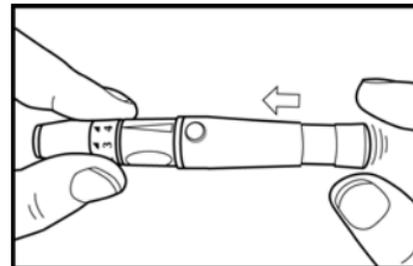

6. Set the lancing device aside until later in the test.



1. **Select 1-2 for soft or thin skin, 3 for average, and 4-5 for thick or calloused skin.**
2. **Lancing device and lancets are not to be shared between users. Sharing lancing devices and lancets may transmit blood borne pathogens, such as viral hepatitis.**


Running A Blood Glucose Test With Blood From Your Fingertip



1. Wash your hands with soap and warm water. Rinse and dry thoroughly.




2. Put a test strip into the meter in the direction of the arrow. The meter turns on.

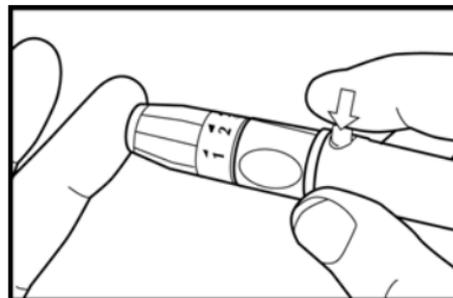

3. Swab the blood collection area on your finger with an alcohol swab. Please wait at least 5 seconds until the intended area is dry and clean before sampling the blood.
4. Place the lancing device against the pad of your finger. Press the trigger button to activate the lancing device.



If a flag icon of “” is set, press “” for 1 seconds to cancel the setting of control solution test.

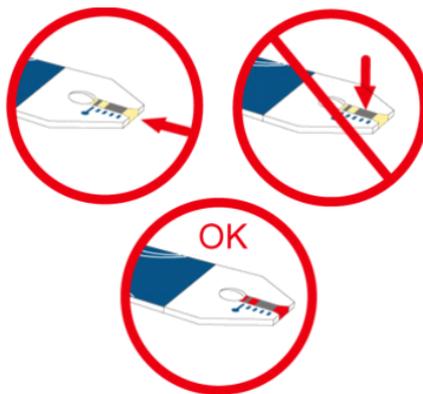


5. When the blood drop flashes on the display, obtain a drop of blood from your fingertip.

6. Gently squeeze your finger to assist the flow of blood. This helps you get a blood drop.
Touch the drop to the tip of the transparent window of the test strip.
Do not put blood on top of the strip. Be sure to get enough blood on the strip's reaction zone.
Otherwise, an inaccurate reading may result.


7. The meter will beep when enough blood has entered the strip's reaction zone.
The result will appear on the display after 5 seconds.

Running A Blood Glucose Test With Blood From Your Forearm


Please use the clear cap with the lancing device for AST testing.

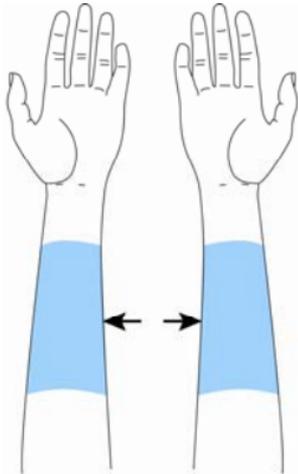

1. Massage the puncture area of forearm or forearm for a few seconds.

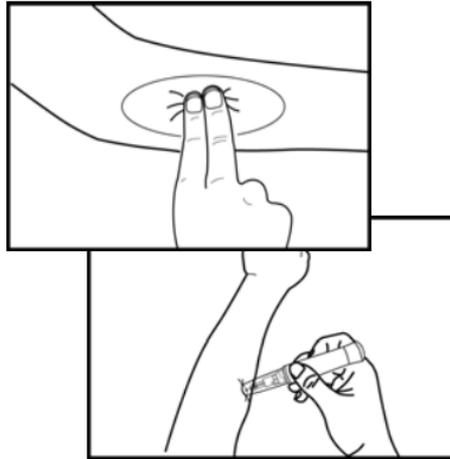


2. Press and hold the device with clear adjustable tip against the forearm.

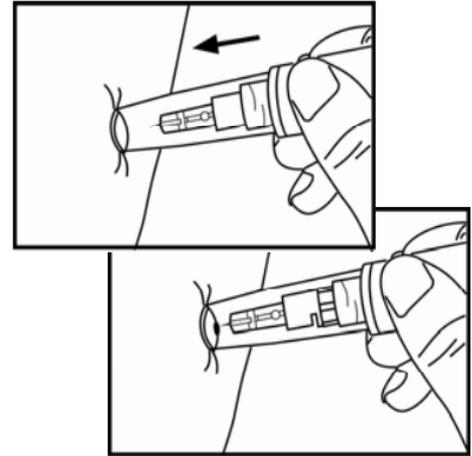


3. Press the trigger button to activate the lancing device.
4. Hold the device against forearm and increase pressure until the blood sample size is sufficient.


Running a Blood Glucose Test with Blood from Your Palm

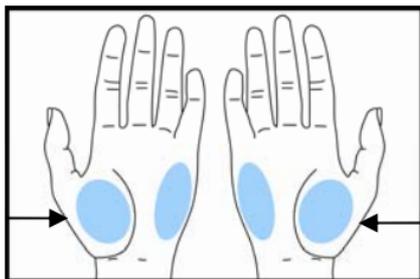

1. Massage the puncture area of palm for a few seconds.

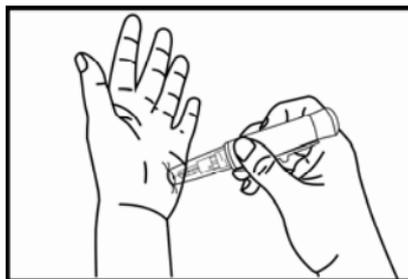

2. Press and hold the device with one clear adjustable tip against the palm.

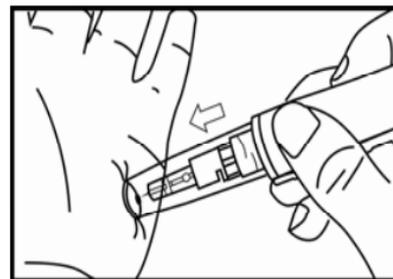


3. Press the trigger button to activate the lancing device.

4. Hold the device against palm and increase pressure until the blood




Check with your healthcare professional before testing other sites than fingertip.


Discarding Used Lancets

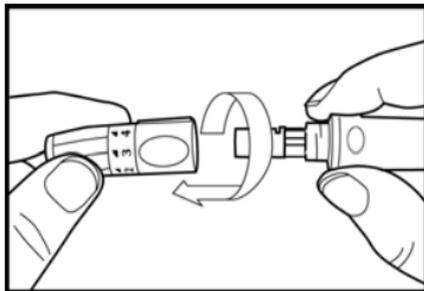

1. Unscrew and remove the cap.

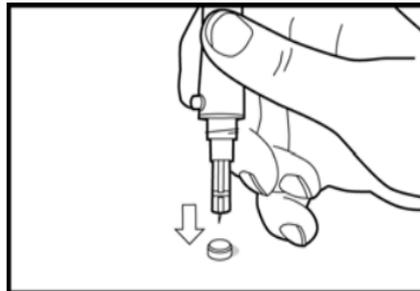


2. Without touching the used lancet, stick the lancet tip into its protective cover.

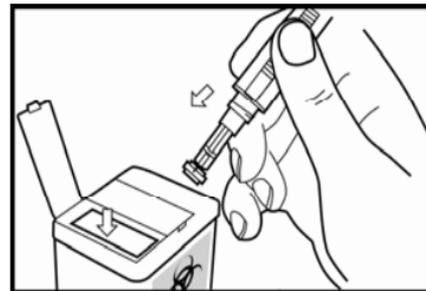

3. Pointing the lancing device toward a container for sharp or biohazard material, slide the ejection button down to release the covered lancet into the container.


Viewing Test Results

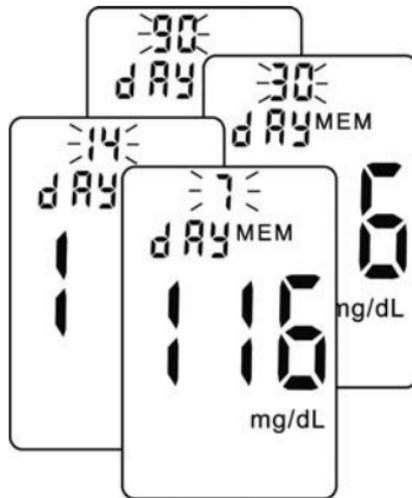


1. Press "▶" to view the last test result.
2. Press "◀" to view the previous results in order from the latest to the earliest.
3. Press "▶" once again to view averages of 7-day test result.
4. Press "◀" to review averages of 14-day, 30-day and 90-day test results.
5. Press "▶" to be back to the testing mode of flashing strip.

Setting The Alarm


The meter can set up to 4 alarms, allowing you to control your test times according to your requirements.

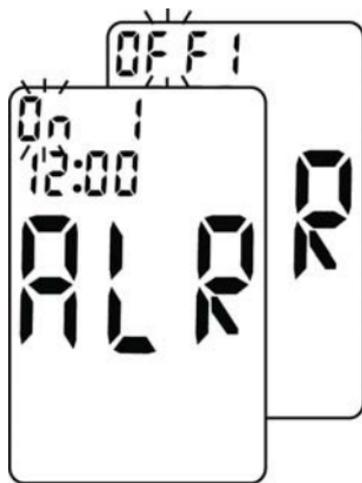

1. Press "▶" for 5 seconds and enter the setting mode of alarm.
2. Press "◀" to set "On" for the first alarm.
3. Press "◀" to adjust time and press "▶" to confirm the setting (24-hour clock).

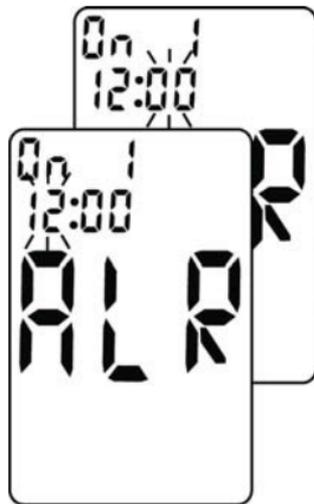

4. Press "▶" to confirm the first setting and then get into the second one.

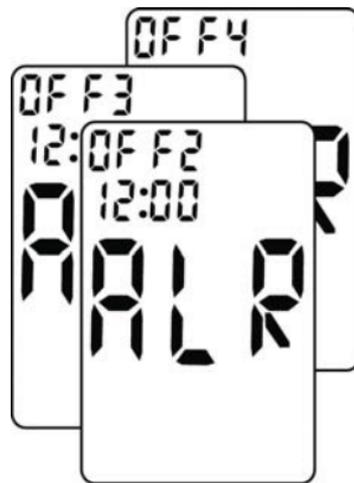

5. Repeat step 1 to 4 to set other 3 alarm. If you don't want to turn on the alarm at all, turn every alarm "OFF" at the upper left corner of the display. Press "▶" to confirm the setting.

Screen Messages And Troubleshooting

Never make treatment decisions based on an error message. If you have any concerns, please contact your local dealer.



Humidified / Used strips

Action: Replace with a new strip.



Low power

Action: Replace with new batteries.



System fault

Action: Replace the batteries first. If 001 ERROR appears again, please contact your local dealer.



System fault

Action: Replace the batteries first. If 005 appears again, please contact your local dealer.



The "Ht" and thermometer icon appears. Temperature is too high, outside the required range of 10°C ~40°C (50°F ~104°F). This alerts users that an incorrect result may occur if the test continues.

Action: Relocate the meter to a location with temperature between 10°C ~40°C (50°F ~104°F).



The "Lt" and thermometer icon appears. Temperature is too low, outside the required range of 10°C ~40°C (50°F ~104°F). This alerts users that an incorrect result may occur if the test continues.

Action: Relocate the meter to a location with temperature between 10°C ~40°C (50°F ~104°F).



Err message.
**Not enough sample
was drawn into the test
strip for measurement.**
Action: Discard the test
strip and repeat the test.



**Test result is higher than
600 mg/dL.**
Action: Test again. If the
result is still the same,
please contact your
healthcare professional.



**The test result is lower
than 20 mg/dL.**
Action: Test again. If the
result is still the same,
please contact your
healthcare professional.



**Manufacturer:
EPS BIO TECHNOLOGY CORP.**

No.8, R&D RD. III, Hsinchu Science Park, Hsinchu, Taiwan 30077

TEL : +886-3-6686868 FAX : +886-3-6686866

E-mail : info@epsbio.com.tw Website : <http://www.epsbio.com.tw>



Obelis s.a.

34, Av. de Tervuren, bte 44, B-1040 Brussels, Belgium

TEL : (32) 2.732.59 54 FAX : (32) 2.732.60 03

E-mail: mail@obelis.net